


## ALPHA ACTIVE 4 MATTRESS REPLACEMENT – ISCHIAL

**Alpha Active®4 Mattress Replacement  
Interface Pressure On Right Ischial of 86kg, 1.75m Male Subject**

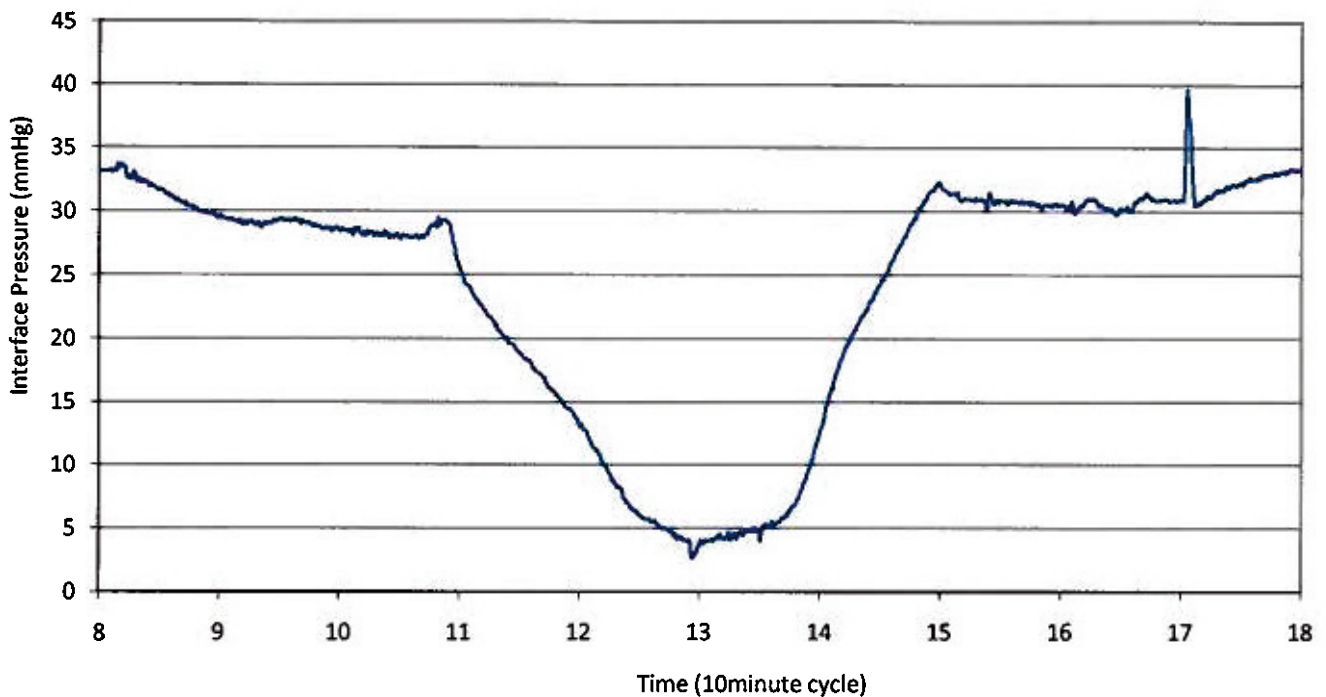

**Note:** This example represents test results from one individual only and different results may occur with different subjects. Only large scale tests can determine true performance differences.

© is a trademark belonging to ArjoHuntleigh group of companies.

ArjoHuntleigh is a branch of Arjo Ltd Med. AB. Only ArjoHuntleigh designed parts, which are designed specifically for the purpose, should be used on the equipment and products supplied by ArjoHuntleigh. As our policy is one of continuous development we reserve the right to modify designs and specifications without prior notice. © and ™ are trademarks belonging to the ArjoHuntleigh group of companies.  
© ArjoHuntleigh, 2008

T.S.FRI.03.0.GE-INT.0

### Therapy & Prevention Product Division

ArjoHuntleigh House, Houghton Hall Business Park, Houghton Regis, Bedfordshire, LU5 5XF, UNITED KINGDOM

• Phone: +44 (0) 1582 413104 • Fax: +44 (0) 1582 745745 [www.ArjoHuntleigh.com](http://www.ArjoHuntleigh.com)